



**Yocom-McColl Testing Laboratories, Inc.**  
540 West Elk Place • Denver, Colorado 80216-1823 USA  
PHONE (303) 294-0582 • FAX (303) 295-6944  
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan  
Micron Test Report**

High Plains Alpacas/Rick & Evelyn Derksen  
Site 307, Box 36, R.R. #3  
Saskatoon SK S7K 3J8 Canada

06/26/06

Test No: 278423


**Animal and Sample Description**

**Animal Name:** High Plains Saharan  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** XXXXX

**Animal ID:** XXXXX  
**Sample Location:** Side  
**Sample Date:** 05/15/06  
**Age:** 08/19/04

**Laboratory Data**

**Mean Fiber Diameter:** 20.2 microns  
**Standard Deviation:** 3.7 microns  
**Coefficient of Variation:** 18.3 %  
**Fibers Greater Than 30 microns:** 1.6 %

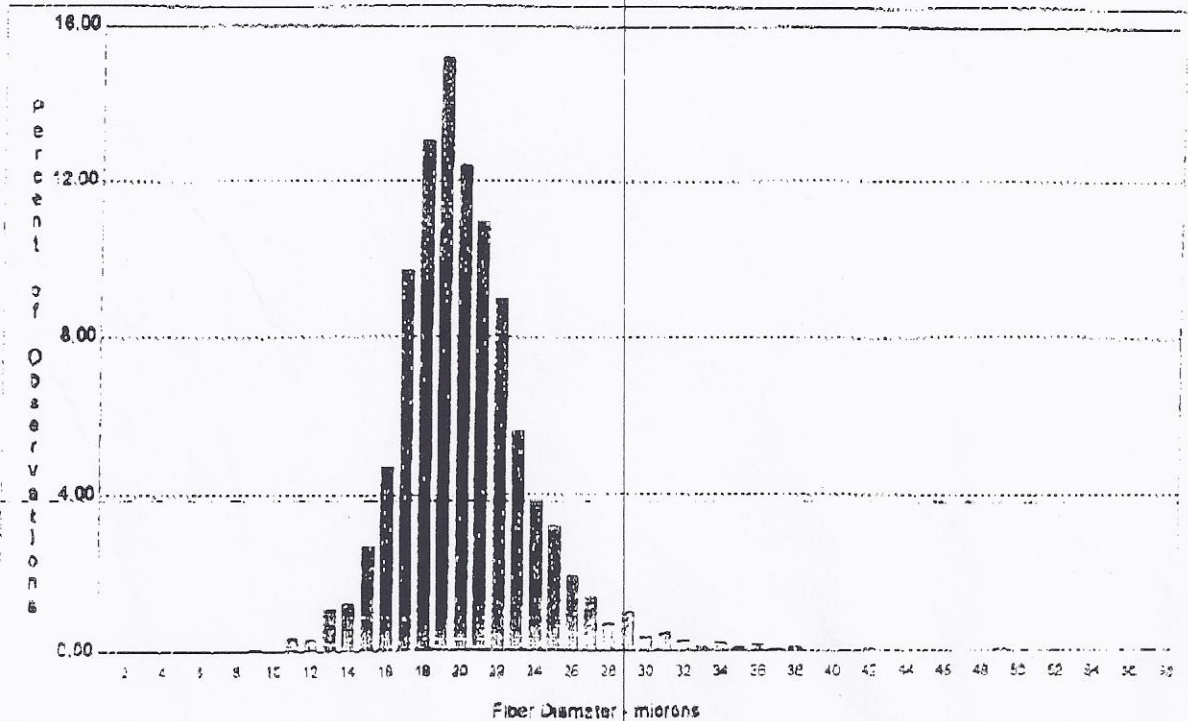

This Test Performed According to I.W.T.O Method 12